



designed for scientists



## Dry Block Heater 1

/// Data Sheet

Digital block heater for one aluminum block provides precise temperature control in small vessels. Included PT-1000 temperature sensor allows temperature control directly in the sample vessel. It is used with PCR tubes, PCR strips, Greiner tubes, microplates and cuvettes. The block heater is ideal for melting and boiling point determination, enzyme reactions, incubation and activation of cultures, immunoassays, DNA denaturation, culture media tests, coagulation tests, blood-urea-nitrogen determinations and in situ hybridizations.

- Stepless adjustable temperature up to 120 °C
- Timer: Countdown, adjustable from 1 min to 99h 59min



designed for scientists

- Counter: Display of heating time
- Highly versatile with a large number of blocks
- Error code display
- Fixed safety circuit
- Acoustic signal at end of test





designed for scientists

## Technical Data

Number of blocks	1
Heat output [W]	165
Heating temperature range [°C]	room temp. +5° - 120
Temperature display	yes
Adjustment and display resolution [K]	1
Connection for ext. temperature sensor	CT (DIN12878)
PT 1000 variation;DIN EN 60751 Kl. A [K]	$\leq \pm (0.15 + 0.002 \times  T )$
Temperature stability within the blocks at 37°C * [°C]	±0.2
Temperature stability within the blocks at 60°C * [°C]	±0.4
Temperature Homogeneity @ 37°C * [K]	0.2
Temperature Homogeneity @ 60°C * [K]	0.4
Heatingrate / Heat up time with external sensor * [K/min]	5
Set-up plate material	Aluminium alloy
Set-up plate dimensions [mm]	96 x 76
Fixed safety circuit [°C]	150
Timer	yes
Time setting range [min]	1 - 5999
* Measured in IKA DBH Testingblock	Refer Manual for more details
Dimensions (W x H x D) [mm]	151 x 73 x 228
Weight [kg]	1.342
Permissible ambient temperature [°C]	5 - 40
Permissible relative humidity [%]	80
Protection class according to DIN EN 60529	IP 21
Voltage [V]	220 - 240
Frequency [Hz]	50/60
Power input [W]	165



designed for scientists



## Dry Block Heater 2

/// Data Sheet

Digital block heater for two aluminum blocks provides precise temperature control in small vessels. Included PT-1000 temperature sensor allows temperature control directly in the sample vessel. It is used with PCR tubes, PCR strips, Greiner tubes, microplates and cuvettes. The block heater is ideal for melting and boiling point determination, enzyme reactions, incubation and activation of cultures, immunoassays, DNA denaturation, culture media tests, coagulation tests, blood-urea-nitrogen determinations and in situ hybridizations.

- Stepless adjustable temperature up to 120 °C
- Timer: Countdown, adjustable from 1 min to 99h 59min



designed for scientists

- Counter: Display of heating time
- Highly versatile with a large number of blocks
- Error code display
- Fixed safety circuit
- Acoustic signal at end of test






designed for scientists

## Technical Data

Number of blocks	2
Heat output [W]	250
Heating temperature range [°C]	room temp. +5° - 120
Temperature display	yes
Adjustment and display resolution [K]	1
Connection for ext. temperature sensor	CT (DIN12878)
PT 1000 variation;DIN EN 60751 Kl. A [K]	$\leq \pm (0.15 + 0.002 \times  T )$
Temperature stability within the blocks at 37°C * [°C]	$\pm 0.2$
Temperature stability within the blocks at 60°C * [°C]	$\pm 0.4$
Temperature Homogeneity @ 37°C * [K]	0.2
Temperature Homogeneity @ 60°C * [K]	0.4
Heatingrate / Heat up time with external sensor * [K/min]	4.5
Set-up plate material	Aluminium alloy
Set-up plate dimensions [mm]	96 x 152
Fixed safety circuit [°C]	150
Timer	yes
Time setting range [min]	1 - 5999
* Measured in IKA DBH Testingblock	Refer Manual for more details
Dimensions (W x H x D) [mm]	151 x 73 x 304
Weight [kg]	1.724
Permissible ambient temperature [°C]	5 - 40
Permissible relative humidity [%]	80
Protection class according to DIN EN 60529	IP 21
Voltage [V]	220 - 240
Frequency [Hz]	50/60
Power input [W]	250



designed for scientists

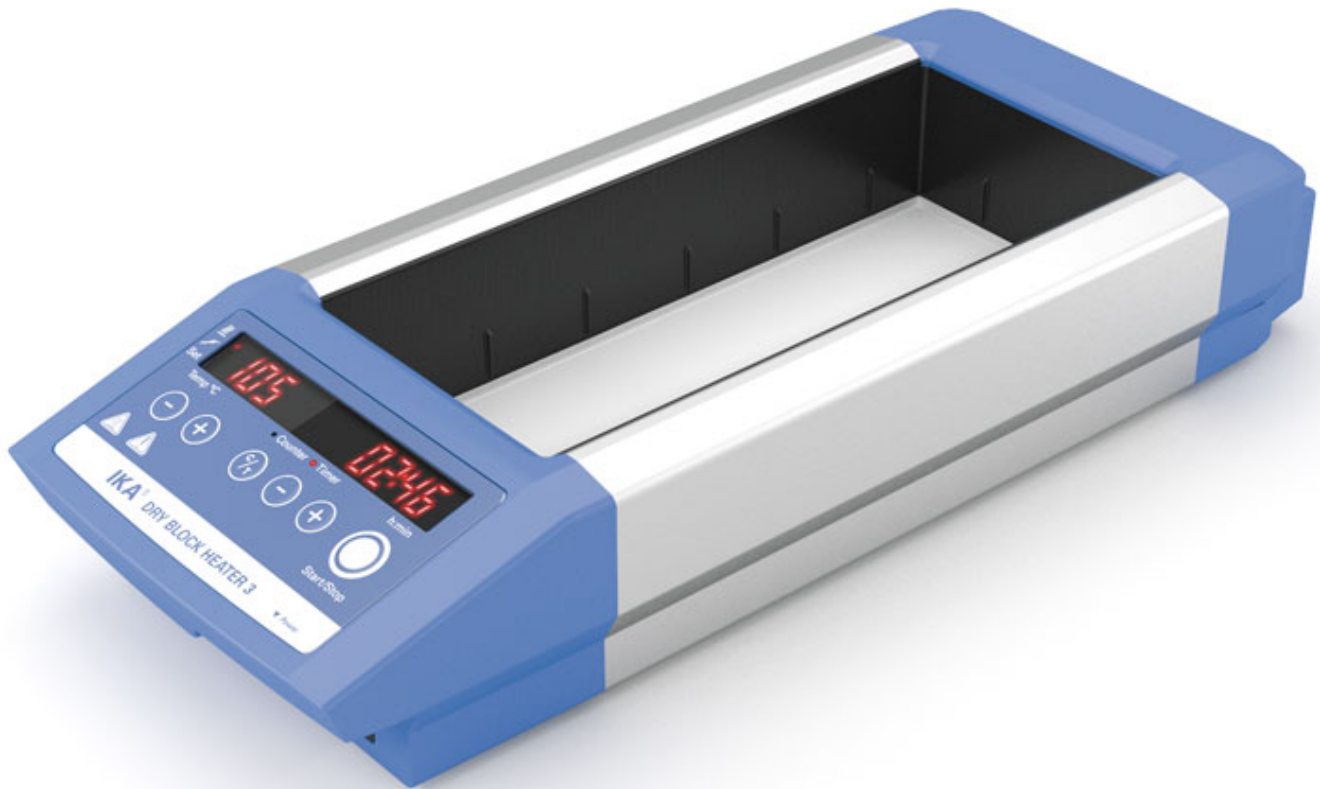

## Dry Block Heater 3

/// Data Sheet

Digital block heater for three aluminum blocks provides precise temperature control in small vessels. Included PT-1000 temperature sensor allows temperature control directly in the sample vessel. It is used with PCR tubes, PCR strips, Greiner tubes, microplates and cuvettes. The block heater is ideal for melting and boiling point determination, enzyme reactions, incubation and activation of cultures, immunoassays, DNA denaturation, culture media test, coagulation test, blood-urea-nitrogen determination and in situ hybridizations.

- Stepless adjustable temperature up to 120 °C
- Timer: Countdown, adjustable from 1 min to 99h 59min
- Counter: Display of heating time



designed for scientists

- Highly versatile with a large number of blocks
- Error code display
- Fixed safety circuit
- Acoustic signal at end of test








designed for scientists

## Technical Data

Number of blocks	3
Heat output [W]	330
Heating temperature range [°C]	room temp. +5° - 120
Temperature display	yes
Adjustment and display resolution [K]	1
Connection for ext. temperature sensor	CT (DIN12878)
PT 1000 variation;DIN EN 60751 Kl. A [K]	$\leq \pm (0.15 + 0.002 \times  T )$
Temperature stability within the blocks at 37°C * [°C]	±0.2
Temperature stability within the blocks at 60°C * [°C]	±0.4
Temperature Homogeneity @ 37°C * [K]	0.3
Temperature Homogeneity @ 60°C * [K]	0.6
Heatingrate / Heat up time with external sensor * [K/min]	4
Set-up plate material	Aluminium alloy
Set-up plate dimensions [mm]	96 x 228
Fixed safety circuit [°C]	150
Timer	yes
Time setting range [min]	1 - 5999
* Measured in IKA DBH Testingblock	Refer Manual for more details
Dimensions (W x H x D) [mm]	151 x 73 x 380
Weight [kg]	2.046
Permissible ambient temperature [°C]	5 - 40
Permissible relative humidity [%]	80
Protection class according to DIN EN 60529	IP 21
Voltage [V]	220 - 240
Frequency [Hz]	50/60
Power input [W]	330



designed for scientists

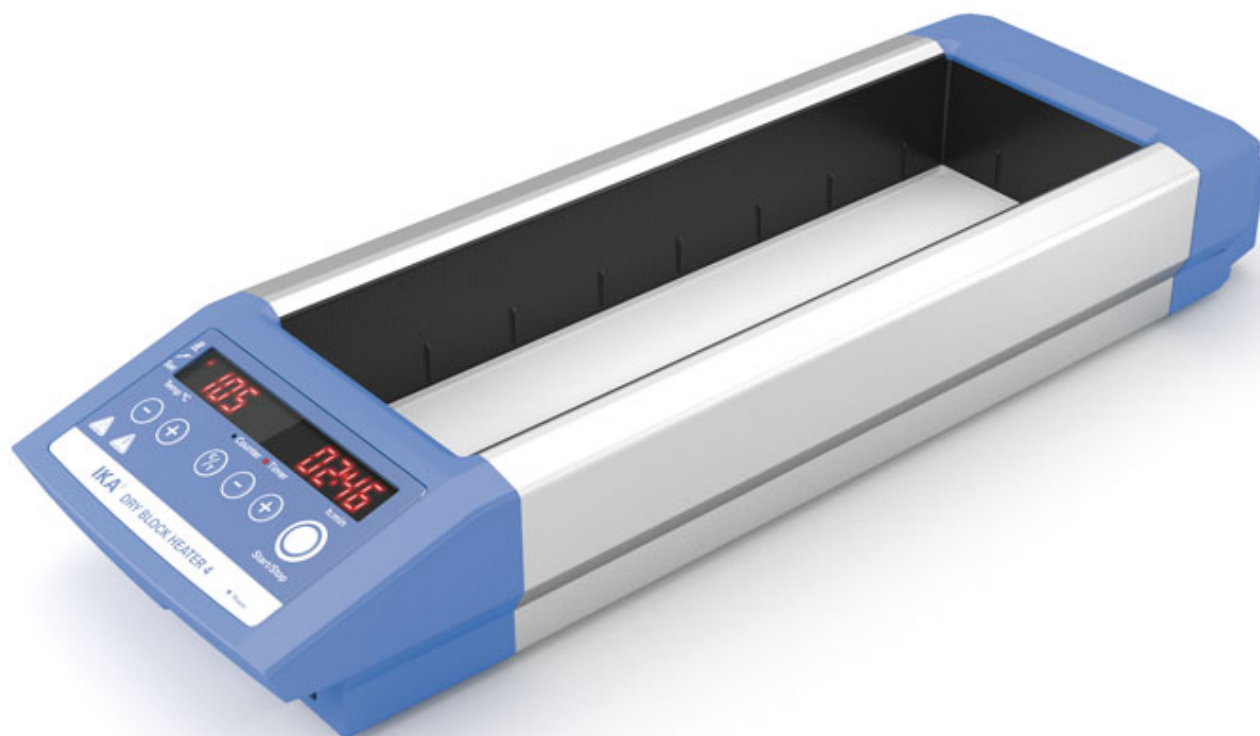

## Dry Block Heater 4

/// Data Sheet

Digital block heater for four aluminum blocks provides precise temperature control in small vessels. Included PT-1000 temperature sensor allows temperature control directly in the sample vessel. It is used with PCR tubes, PCR strips, Greiner tubes, microplates and cuvettes. The block heater is ideal for melting and boiling point determination, enzyme reactions, incubation and activation of cultures, immunoassays, DNA denaturation, culture media tests, coagulation tests, blood-urea-nitrogen determinations and in situ hybridizations.

- Stepless adjustable temperature up to 120 °C
- Timer: Countdown, adjustable from 1 min to 99h 59 min
- Counter: Display of heating time
- Highly versatile with a large number of blocks
- Error code display

[www.ika.com](http://www.ika.com)

Subject to technical changes



IKAworlwide



IKAworlwide /// #lookattheblue



@IKAworlwide



designed for scientists

- Fixed safety circuit
- Acoustic signal at end of test





designed for scientists

## Technical Data

Number of blocks	4
Heat output [W]	412
Heating temperature range [°C]	room temp. +5° - 120
Temperature display	yes
Adjustment and display resolution [K]	1
Connection for ext. temperature sensor	CT (DIN12878)
PT 1000 variation;DIN EN 60751 Kl. A [K]	$\leq \pm (0.15 + 0.002 \times  T )$
Temperature stability within the blocks at 37°C * [°C]	±0.2
Temperature stability within the blocks at 60°C * [°C]	±0.4
Temperature Homogeneity @ 37°C * [K]	0.3
Temperature Homogeneity @ 60°C * [K]	0.6
Heatingrate / Heat up time with external sensor * [K/min]	4
Set-up plate material	Aluminium alloy
Set-up plate dimensions [mm]	96 x 304
Fixed safety circuit [°C]	150
Timer	yes
Time setting range [min]	1 - 5999
* Measured in IKA DBH Testingblock	Refer Manual for more details
Dimensions (W x H x D) [mm]	151 x 73 x 456
Weight [kg]	2
Permissible ambient temperature [°C]	5 - 40
Permissible relative humidity [%]	80
Protection class according to DIN EN 60529	IP 21
Voltage [V]	220 - 240
Frequency [Hz]	50/60
Power input [W]	412